
## VR2 Controller Quick Guide







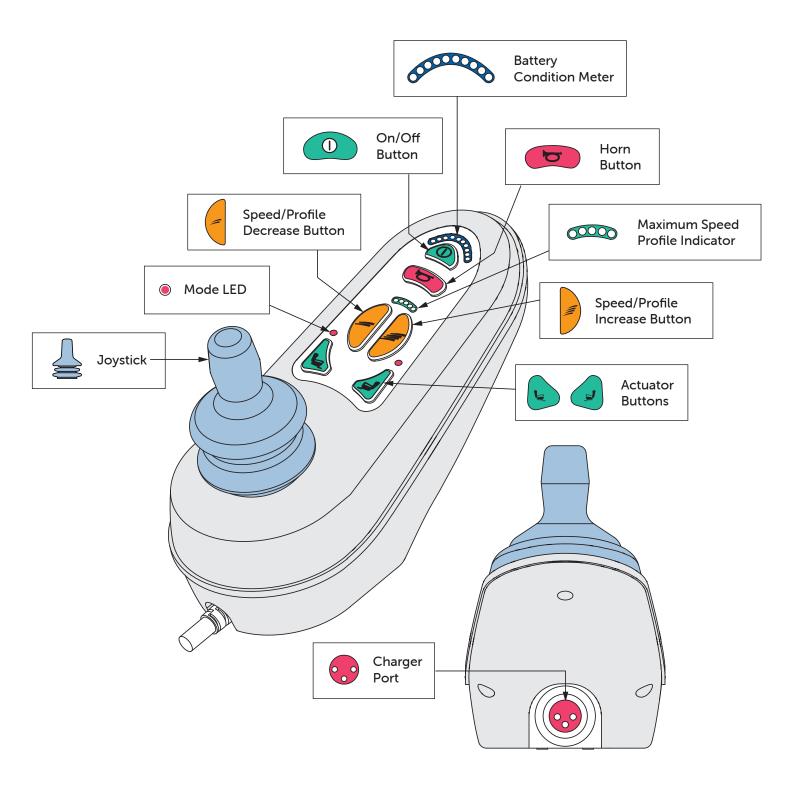

www.alliedmedical.co.nz





## VR2 Controller Quick Guide



Ensure you turn off the powerchair for transfers.




Freewheel your powerchair by disengaging both motors.




Never disengage your motors when on a slope!





**Drive Mode** 




Place unit on level ground and stand to one side when changing between modes.




Remember to charge your powerchair every night.

## **Front View**



Your charger plugs into the front of your hand control.









www.alliedmedical.co.nz

